

AudioControl Room Calibration (ARC) Microphone

We have upgraded the microphone used for Dirac Live calibration. There is no more separate USB sound card, Hurrah!

The splendid new ARC microphone looks like this:



With this new ARC microphone, there is also a new Dirac Live software package which you can download from our website – audiocontrol.com.


There are now two microphone calibration files to choose from within the “Mic config” tab of the Dirac Live for AudioControl software:

One file is for the previous microphone, and the other is for the new ARC microphone.

The new mic calibration file is called “AudioControl_AVRMicCal2.txt”. If you are using the new ARC mic, please make sure you select this new file for best results! The procedure is shown below:


To select the microphone in the Dirac Live program:

Within the “Mic config” tab of the Dirac software, click on the “Recording Device” drop-down menu to select the correct calibration file.

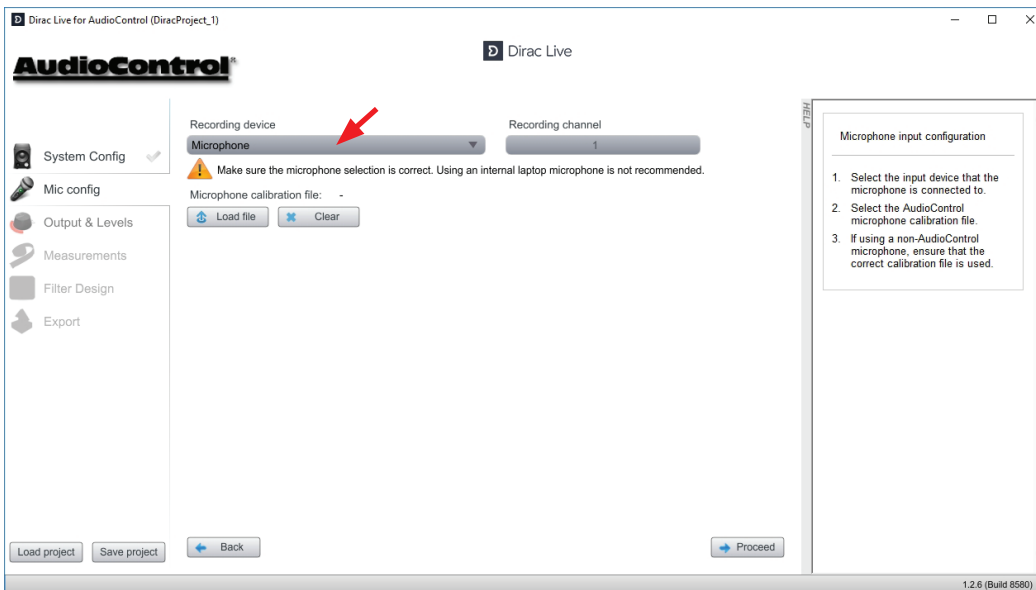


continued...

Using the drop-down menu, select the ARC microphone:

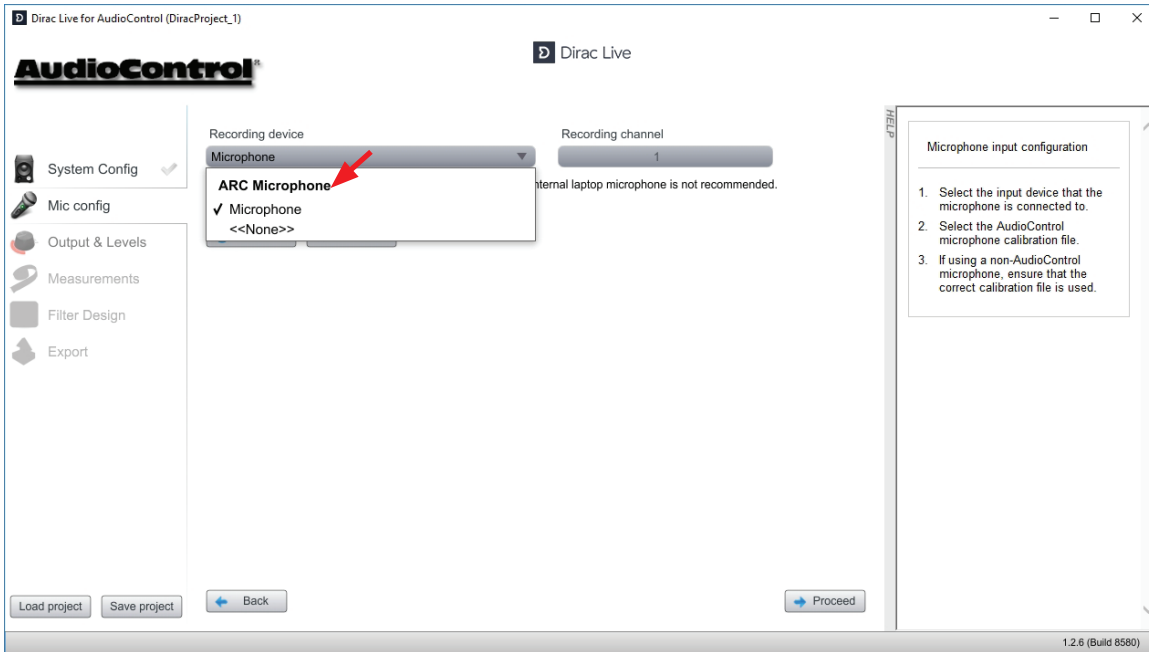

Then click the "Load file" button from the Microphone calibration file option:

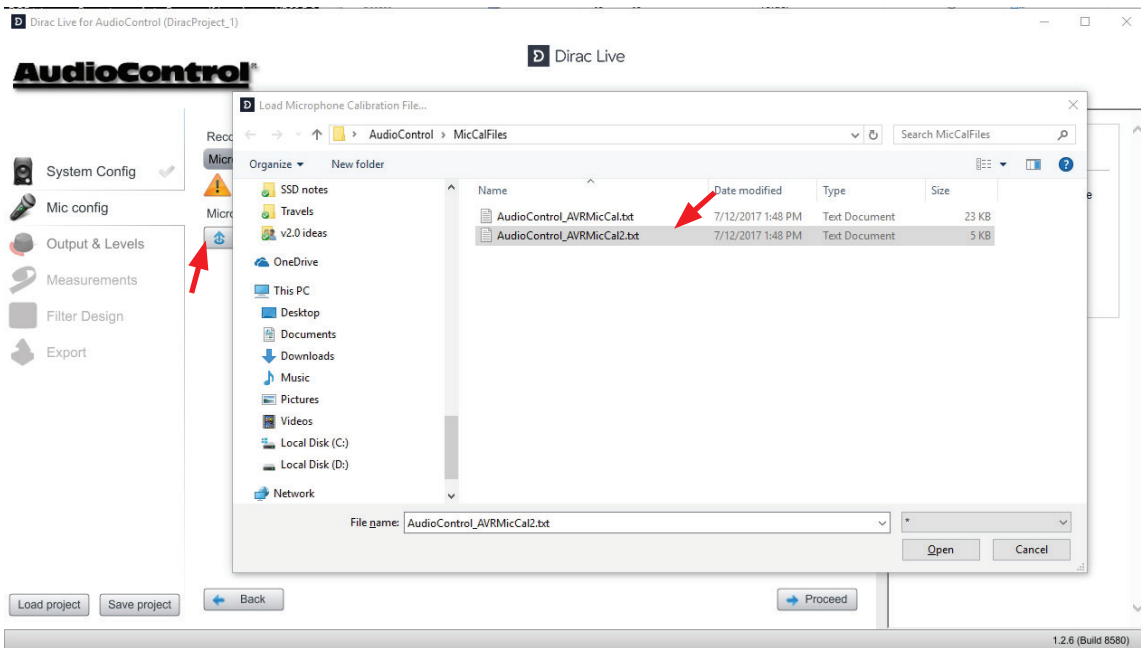

Select the **AudioControl_AVRMicCal2.txt** and you will be all set! Select proceed and move on with your calibration.

AudioControl
22410 70th Avenue West, Mountlake Terrace, WA 98043 USA,
Phone 425-775-8461, FAX 425-778-3166
e-mail: sound.great@audiocontrol.com